

Model HW / 10600-9

OWNER'S MANUAL

Advanced DFS Air Purification System

A tall, white, rectangular air purifier unit with a dark base, standing on a reflective surface. The unit is positioned on the left side of the page.

healthy air |
for all your indoor spaces™

Warranty Registration: Please complete the Warranty Registration today to ensure you receive all the benefits you are entitled to.

Warranty Verification: Registering your product within 10 days of receipt confirms your right to maximum protection under the terms and conditions of your HW/10600-9 Warranty.

Owner Confirmation: Your completed Warranty Registration information serves as verification of ownership in the event of product theft or loss.

Model Registration: It is important to return your Warranty Registration information right away to guarantee you will receive all the information and special offers which you qualify for as the owner of your new Model HW/10600-9.

Please Note:

Your HealthWay® Advanced Air Purifier has been carefully packaged to avoid damage in shipping and storage. **Retain this packaging.**

Before operating air purifier for the first time, open panel and remove plastic bag from carbon/prefilter.

Please inspect your unit to insure that you receive the product free of any visible signs of damage. If you detect any damage, you should file a claim with the shipping company or carrier within 15 days of receipt.

The HealthWay® Advanced Air Purifier is designed for “plug and play” operation and comes complete, ready for use. Simply follow the instructions for set up contained in this owner’s manual.

To receive maximum benefit from the HealthWay® DFS Air Cleaner, we recommend replacing the DFS Main Filter every 12 months and the carbon prefilter every 6 months. For filter replacement orders, please contact place of purchase.

Important Safety Precautions:

Please read all instructions before operating your air cleaner. Basic precautions should always be observed when using electric appliances to reduce the risk of fire, shock and injury.

Observe the following general precautions to insure effective, safe and trouble-free operation of your HealthWay DFS Air Cleaner.

Warning: This air cleaner must be plugged into a 120 or 220 Volt, AC earth grounded outlet. Please refer to unit’s Electrical Specifications located on the rear of the unit before plugging into the wall outlet. Do not use a wall outlet adapter. **Do not operate this air cleaner with an extension cord.**

1. **Plug the unit DIRECTLY** into an earth grounded standard 120 or 220 volt, AC electrical outlet. Insert the plug into the outlet fully. The plug is a polarized line plug (one blade is wider than the other) and can only be inserted one way as a safety feature.
2. **Place the unit on a flat and level surface** to allow continuous airflow to the bottom and side intake and out the top outlet grill.
3. **Always unplug the air cleaner** before moving it, opening the front panel, changing the main filter, changing the carbon prefilter or before cleaning. (Clean only with a dry, non-static cloth.)
4. **Do not place any foreign objects inside the unit** because electric shock and injury could result.
5. **Do not use the unit if any part is missing** or damaged in any way.
6. **Do not run power cord under carpeting or near heaters, registers, radiators, stoves or fireplaces.** To avoid a tripping hazard, keep the power cord away from traffic areas.
7. **Never operate the air cleaner in areas where combustible gases** or vapors are present or any other flammable materials.
8. **Never immerse the unit in water or other liquids**, or spray the air cleaner with liquids or clean the air cleaner under running water.

Important Safety Precautions *(continued)*

9. **The air purifier is designed for indoors**, do not use this air purifier outdoors.
10. **Do not operate this unit with a damaged cord or plug**, or after the unit malfunctions or has been damaged in any manner. Call HealthWay® Customer Service at 1-800-843-3860 for servicing instructions.
11. **This unit is designed for residential use only. Do not use in industrial or commercial applications.**
12. **A short power supply cord is provided** to reduce the risk resulting from becoming entangled in or tripping over a long cord. Do not use extension cords with this unit.

WARNING!!! To prevent fire or shock hazard, DO NOT expose this unit to rain or moisture.


Specifications


| | | | |
|------------------------|--|-----------|-----------|
| Model | HW / 10600-9 | | |
| Voltage/Frequency | 120V/60Hz | 220V/50Hz | 220V/60Hz |
| Speeds | High | Medium | Low |
| Power consumption (w)* | 120V/60Hz | 45 | 40 |
| | 220V/50Hz | 40 | 35 |
| | 220V/60Hz | 55 | 45 |
| Operation noise (dB) | 60 | 50 | 40 |
| Dimensions (L x W x H) | 11.22 x 15.16 x 23.23 inches (285 x 385 x 590mm) | | |
| Weight | 17 lbs. (8kg) | | |

• The Power Consumption in the standby state (operation terminated) is about 1.2 watts.


Usage

■ Power On





- Press the button  and the purifier automatically runs on high speed. Each time you press the power button the operation mode will systematically change to the next speed.




Indicator:



Function:



- To turn off the purifier, keep pressing the  button until the purifier powers off.

■ DFS Indicator Light


- When air purifier is in normal operation mode, the advanced purification system indicator light will be on. This indicates system is working properly.
- The **DFS** indicator light flashes when the advanced **DFS** filter needs to be replaced.

Maintenance


NOTE: Turn off air purifier and unplug from the power outlet before installing or replacing filters.

Replacement Filters: Please call your dealer or place of air system purchase to attain filter replacements.


■ Advanced DFS Filter installation instructions.

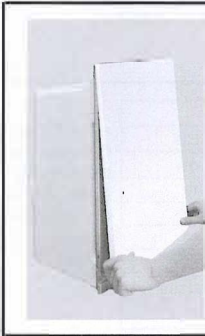


1. Turn off air purifier and unplug it from power outlet, then open and remove the front panel.

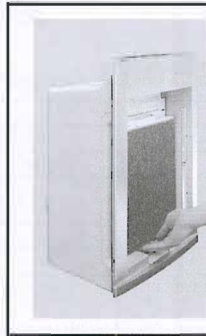


2. Take out Prefilter. Clean or vacuum Prefilter every month removing the large dust off the filter.

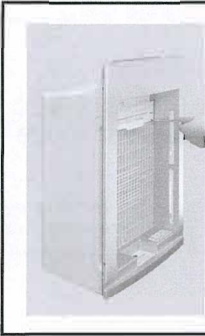


3. Unscrew housing holding DFS filter in place with a screwdriver.

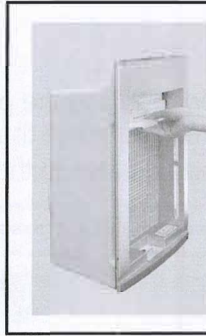

4. Pull out dirty DFS filter carefully and discard properly. Pop in new filter securely.

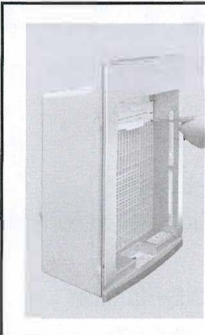


5. Using a screwdriver firmly screw filter housing in place, OR remove wing nut holding filter in place.

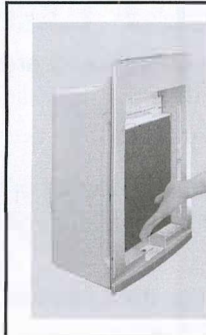

6. After vacuuming large dust off of Carbon Prefilter, carefully insert prefilter back into unit and put front panel back on.

■ Maintenance *Continued*

■ After Replacing Advanced DFS Filter

- Please put used filter in opened filter bag before discarding.
- Reset timer after replacing filter:
 - Plug unit directly into working outlet and let it run on HI.
 - Press the  (Power Button) down for 10 seconds or until DFS indicator light turns on.

■ Clean Prefilter:

- Prefilter/Carbon Filter must be replaced every 6 months in order for air cleaner to work at its full potential.
- The prefilter also can be cleaned monthly if the environment is dusty.
- Before cleaning prefilter, turn off unit and unplug from wall. Open front panel and gently pull out prefilter, the front panel pulls out at top.
- You may gently vacuum prefilter to remove the large dust off the filter.

■ Regular Maintenance:

- Clean housing/exterior surface with a soft clean slightly dampened cloth. Use water only.
- NO CLEANING AGENTS are to be used on this unit!

■ Trouble Shooting Guide

■ Unit Will Not Turn ON:

- Is unit plugged into "working" AC earth ground outlet?
- Is the unit's front panel in place, and front panel is snapped shut securely?
- Are the filters securely in place and seated correctly?




If unit will not turn on after trying the above, or the unit will not change speed, please call HealthWay Customer Service.

■ DFS Filter Light is Flashing or is Not On:

- Replace DFS Filter-must be replaced no later then 12 months or earlier depending on environment. Replace Prefilter/Carbon Filter every 6 mos.
- If unit does not start after replacing filters and checking filters seating, call HealthWay's Customer Service at 1-315-298-2904.

- Listed as a FDA Class II Medical Device
- Certifications: ETL&CE
- Manufactured in our facilities under strict ISO9001: 2008 International quality standards and guidelines
- Each unit individually tested

Parts and Functions

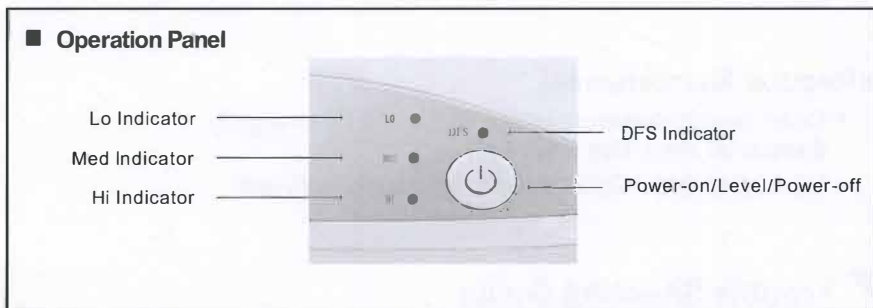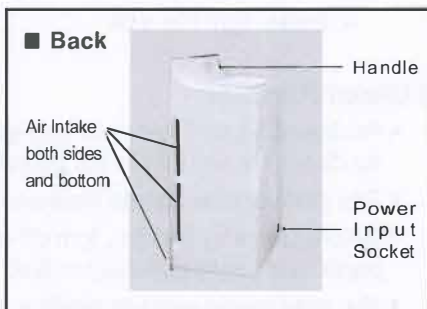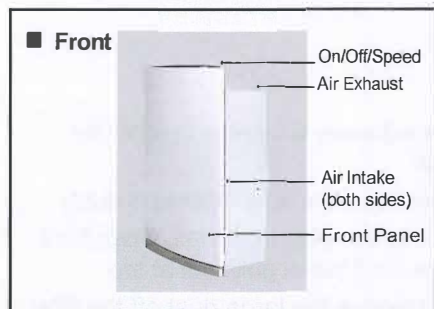

WARNING ! To prevent fire or shock hazard, DO NOT expose this unit to rain or moisture.

HealthWay® Offers a One-Year Limited Warranty

- 1) You must retain proof of purchase and the original box and packaging material.
- 2) The Warranty Registration Card must be mailed or faxed within 10 days from original purchase date.

To make a Warranty Product Claim, please call 1-315-298-2904 to obtain a Warranty Claim Number. You must have this number before sending product to us for warranty work.

Product Registration:

HealthWay® makes this 1-Year Limited Warranty ONLY to original retail purchaser who completes the enclosed Warranty Registration Card within 10 days of purchase and sends or faxes it to them at HealthWay Products, 3420 Maple Ave., PO Box 485, Pulaski, NY 13142 - Ph. 1-315-298-2904 / FAX 315-298-6992

This Limited Warranty applies only to the repair or replacement of any manufactured or supplied part of this product which, upon inspection by HealthWay® authorized personnel, proves to have failed in normal use due to defects in material or workmanship. The sole responsibility of HealthWay® under this Limited Warranty is, in its sole discretion, to either repair or replace a duly registered product (or defective part thereof) with the same or a comparable model within a reasonable period of time, subject to the following exclusions, limitations, statutory rights, and warranty claim procedures. This Limited Warranty is exclusive, and HealthWay® expressly disclaims all other or additional warranties, whether written or oral, expressed or implied, including, but not limited to, warranties of merchantability, workmanship, or fitness for a particular purpose.

Exclusions:

- A.** This Limited Warranty does not apply, or is void, as to any product or part damaged by (1) accident, misuse, abuse, or lack of reasonable care or normal maintenance; (2) installation or operation under conditions other than those recommended by HealthWay®; (3) subjecting the product to any but the specified voltage; (4) servicing or disassembly by unauthorized personnel; (5) removing or defacing the serial number; or (6) modifying the original factory-assembled unit in any way.
- B. THIS LIMITED WARRANTY DOES NOT APPLY TO SHIPPING CHARGES FOR PRODUCT SHIPPED TO OR FROM THE FACTORY OR DESIGNATED SERVICE CENTER IN CONNECTION WITH WARRANTY CLAIMS NOR DOES IT APPLY TO ANY DAMAGES OCCURRING DURING SUCH SHIPMENT.**
- C.** This Limited Warranty does not apply to installation, removal, reinstallation, and/or related expenses.
- This Limited Warranty does not apply to replaceable filters.**

Limitations:

HealthWay® shall not be liable for property, incidental, and/or consequential damages of any kind and, unless otherwise prescribed by applicable state law, HealthWay® shall not be liable for personal injury resulting from malfunctions, defects, misuse, improper operation or installation, or alteration of a HealthWay® product or any part thereof. The exclusive remedy for a breach of this Limited Warranty is the repair or replacement of the defective product. In no case, shall liability under any other remedy prescribed by law exceed the purchase price of the product,

Warranty Claims Procedure:

The validity of a product claim under this Limited Warranty depends upon following these simple steps. **To make a product claim, please follow steps A-D:**

- A. Contact Warranty Claim Dept.:** Call HealthWay Products™ Customer Service at 315-298-2904 or 1-800-843-3860 to make a warranty claim.
- B. Packaging and Shipping:** Upon instructions from HealthWay™ customer service/warranty department, carefully pack the product in its original carton with original packaging materials or comparable box and materials to avoid damage in shipping. For convenience in tracking your shipment, HealthWay™ recommends that you ship the unit by United Parcel Service (UPS). **ALL OUTBOUND AND RETURN WARRANTY PRODUCT SHIPPING CHARGES MUST BE PREPAID BY YOU.**

HealthWay™ cannot accept freight collect shipments.

- C. Assemble and Enclose Information:** Enclose the following information in an envelope and tape the envelope to the unit itself:
- (1) your Warranty Claim Number
 - (2) your name, complete address with zip code, and telephone number
 - (3) a dated sales receipt or dated Proof of Purchase; and
 - (4) a short specific description of the malfunction

- D. Ship the Product Prepaid to:**
Warranty Claim Department
Warranty Claim Number _____

HealthWay Products, Inc.
PO Box 485
3420 Maple Avenue
Pulaski, NY 13142

This Shipping Address and the Warranty Claim Number must, *without exception*, appear on the outside of the shipping carton.

®

